



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Rainbow Forest Acres/Barbara & Daniel Eslake
P.O. Box 1203
Mt. Currie BC V0N 2K0 Canada

06/14/10

Test No: 375132


Animal and Sample Description

Animal Name: RFA Anise
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/01/10
Age: 08/2007

Laboratory Data

Mean Fiber Diameter:	22.0 microns	Spin Fineness:	21.3 microns
Standard Deviation:	4.6 microns	Mean Curvature (deg/mm):	36.4
Coefficient of Variation:	20.8 %	SD Curvature (deg/mm):	20.8
Fibers Greater Than 30 microns:	3.9 %	Comfort Factor:	96.1 %
Medullated Fibers:	6.6 %		

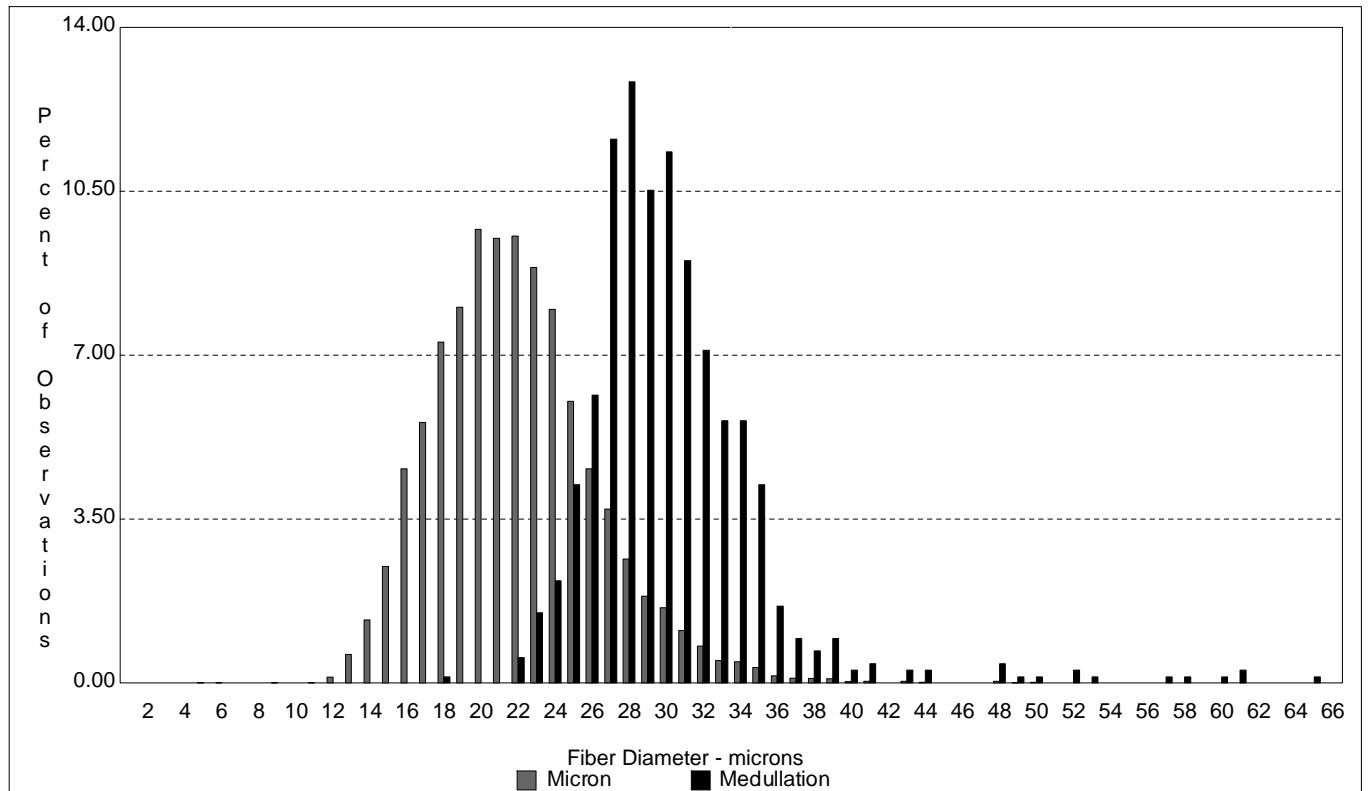

This Test Performed According to I.W.T.O Method 47