



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Rainbow Forest Acres/Barbara & Daniel Eslake
P.O. Box 1203
Mt. Currie BC V0N 2K0 Canada

06/14/10

Test No: 375135


Animal and Sample Description

Animal Name: RFA Cadence
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/01/10
Age: 06/2009

Laboratory Data

| | | | |
|--|--------------|---------------------------------|--------------|
| Mean Fiber Diameter: | 15.8 microns | Spin Fineness: | 16.1 microns |
| Standard Deviation: | 4.1 microns | Mean Curvature (deg/mm): | 52.6 |
| Coefficient of Variation: | 25.8 % | SD Curvature (deg/mm): | 29.5 |
| Fibers Greater Than 30 microns: | 1.1 % | Comfort Factor: | 98.9 % |
| Medullated Fibers: | 2.0 % | | |

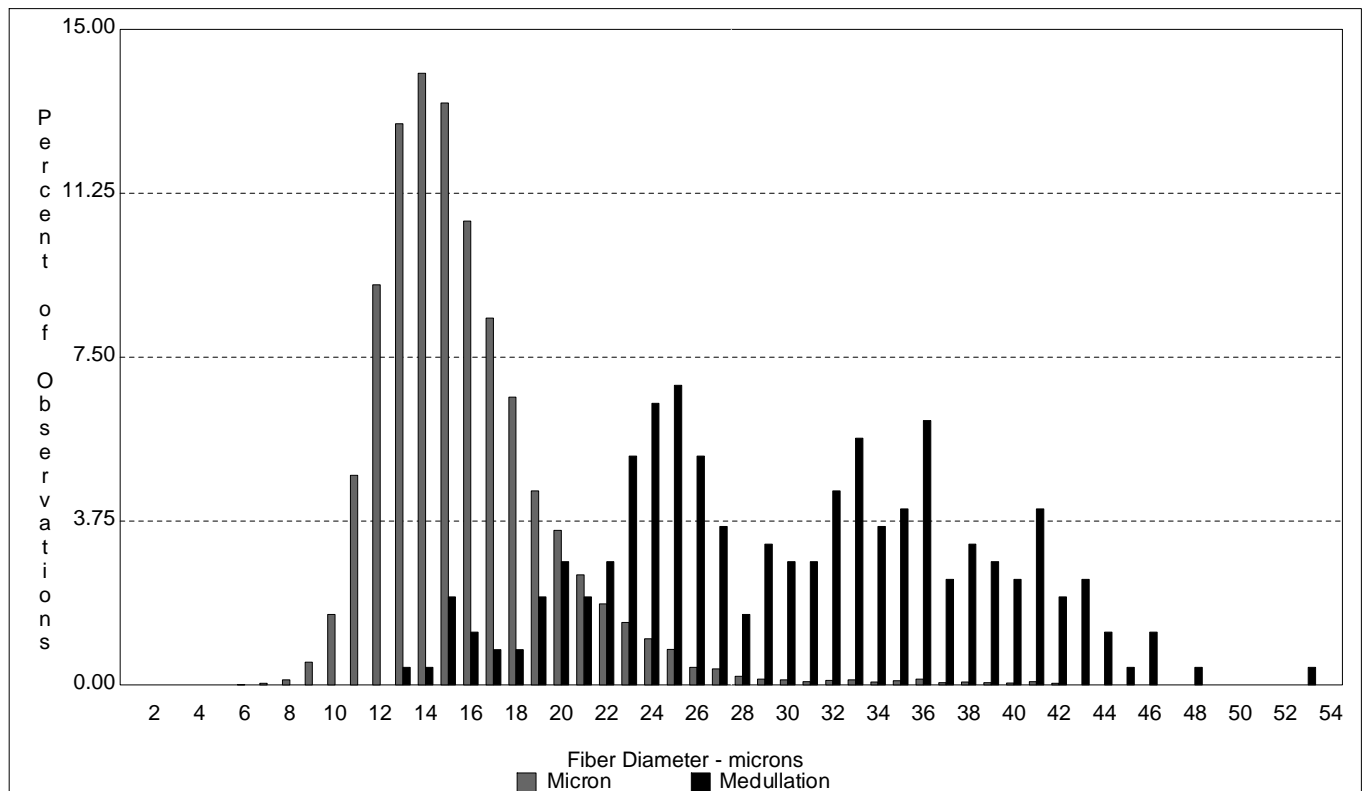

This Test Performed According to I.W.T.O Method 47