



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Rainbow Forest Acres/Barbara & Daniel Eslake
P.O. Box 1203
Mt. Currie BC V0N 2K0 Canada

06/14/10

Test No: 375143


Animal and Sample Description

Animal Name: RFA Chocolate Kisses
Breed: Alpaca(Huacaya)
Sex: Female
Color: Brown

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/01/10
Age: 09/2009

Laboratory Data

Mean Fiber Diameter:	19.8 microns	Spin Fineness:	19.5 microns
Standard Deviation:	4.4 microns	Mean Curvature (deg/mm):	30.6
Coefficient of Variation:	22.4 %	SD Curvature (deg/mm):	21.3
Fibers Greater Than 30 microns:	2.2 %	Comfort Factor:	97.8 %

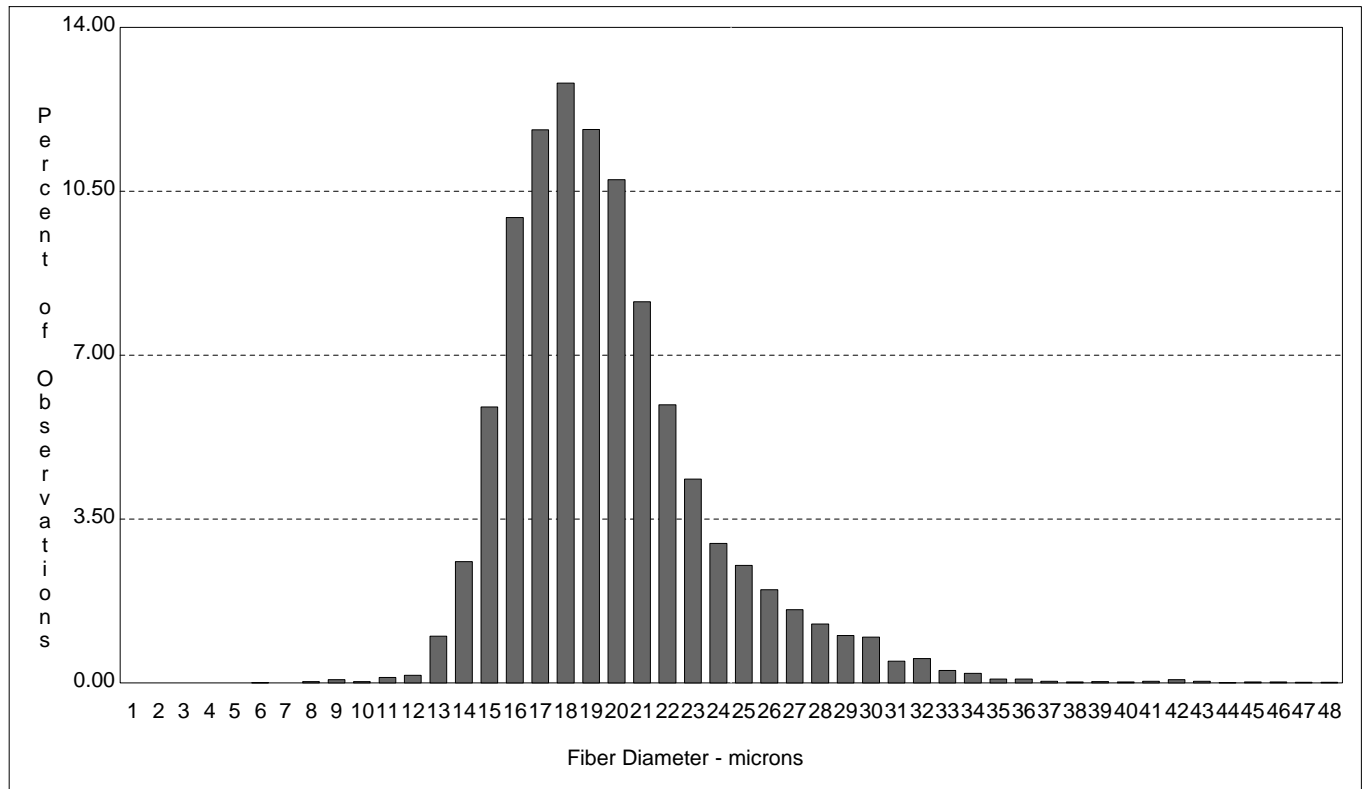

This Test Performed According to I.W.T.O Method 47