



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Rainbow Forest Acres/Barbara & Daniel Eslake
P.O. Box 1203
Mt. Currie BC V0N 2K0 Canada

06/14/10

Test No: 375157


Animal and Sample Description

Animal Name: RFA Damoclese
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/01/10
Age: 10/2007

Laboratory Data

Mean Fiber Diameter:	21.2 microns	Spin Fineness:	20.5 microns
Standard Deviation:	4.3 microns	Mean Curvature (deg/mm):	45.7
Coefficient of Variation:	20.1 %	SD Curvature (deg/mm):	25.7
Fibers Greater Than 30 microns:	2.8 %	Comfort Factor:	97.2 %
Medullated Fibers:	11.3 %		

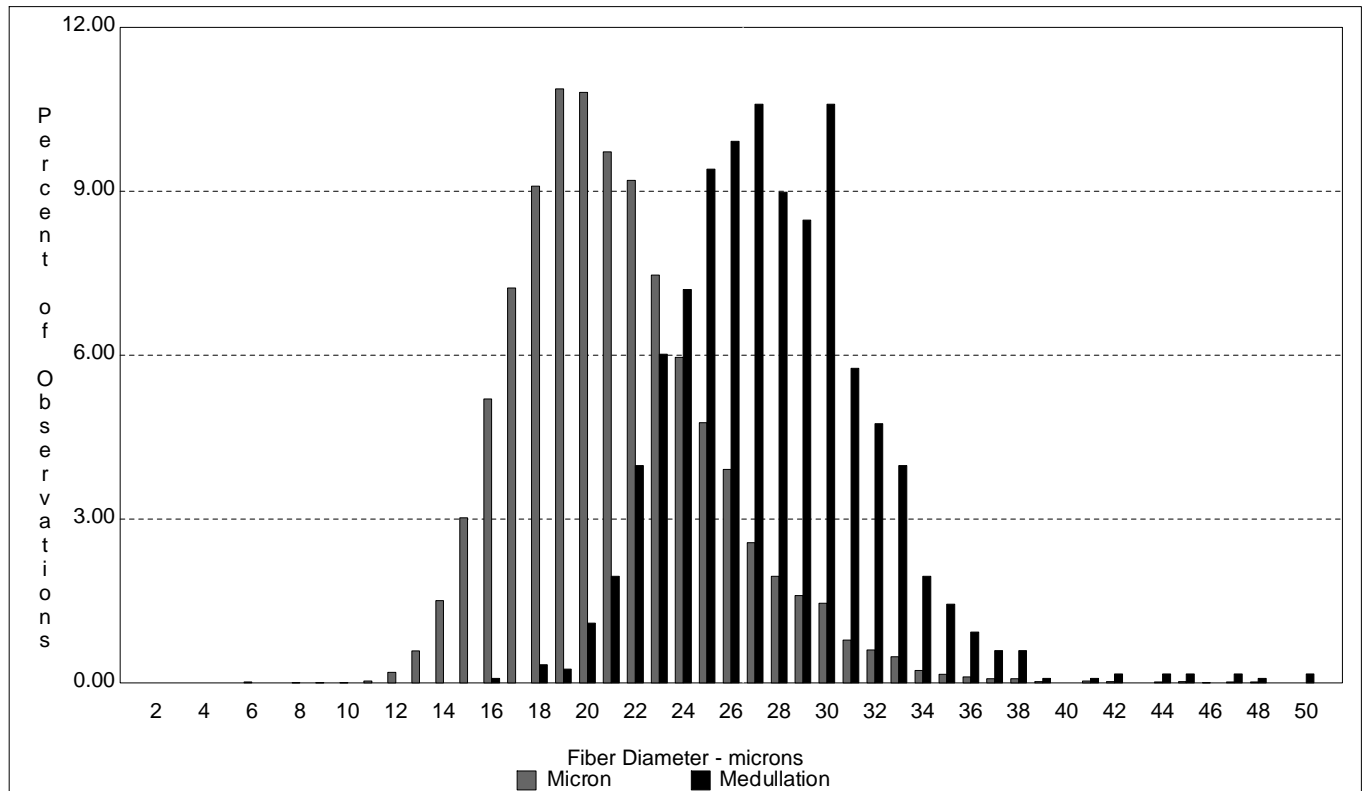

This Test Performed According to I.W.T.O Method 47