



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Rainbow Forest Acres/Barbara & Daniel Eslake
P.O. Box 1203
Mt. Currie BC V0N 2K0 Canada

06/14/10

Test No: 375145


Animal and Sample Description

Animal Name: RFA Lady Guinevere
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/01/10
Age: 05/2006

Laboratory Data

Mean Fiber Diameter:	24.9 microns	Spin Fineness:	23.5 microns
Standard Deviation:	4.4 microns	Mean Curvature (deg/mm):	35.3
Coefficient of Variation:	17.6 %	SD Curvature (deg/mm):	22.9
Fibers Greater Than 30 microns:	8.8 %	Comfort Factor:	91.2 %
Medullated Fibers:	5.2 %		

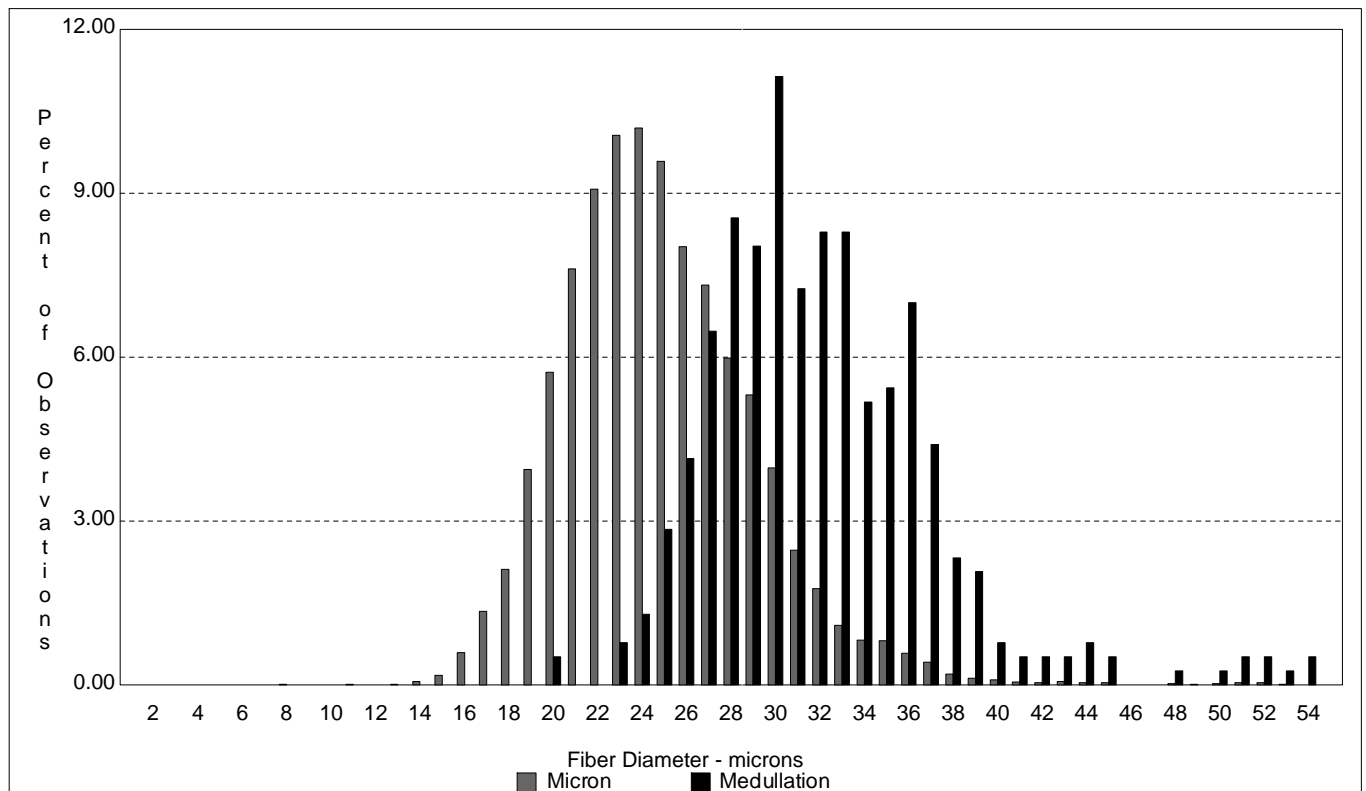

This Test Performed According to I.W.T.O Method 47