



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Rainbow Forest Acres/Barbara & Daniel Eslake
P.O. Box 1203
Mt. Currie BC V0N 2K0 Canada

06/14/10

Test No: 375161


Animal and Sample Description

Animal Name: RFA Shahtzie
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/01/10
Age: 08/2009

Laboratory Data

Mean Fiber Diameter:	19.2 microns	Spin Fineness:	18.3 microns
Standard Deviation:	3.5 microns	Mean Curvature (deg/mm):	45.0
Coefficient of Variation:	18.4 %	SD Curvature (deg/mm):	28.0
Fibers Greater Than 30 microns:	0.7 %	Comfort Factor:	99.3 %
Medullated Fibers:	2.9 %		

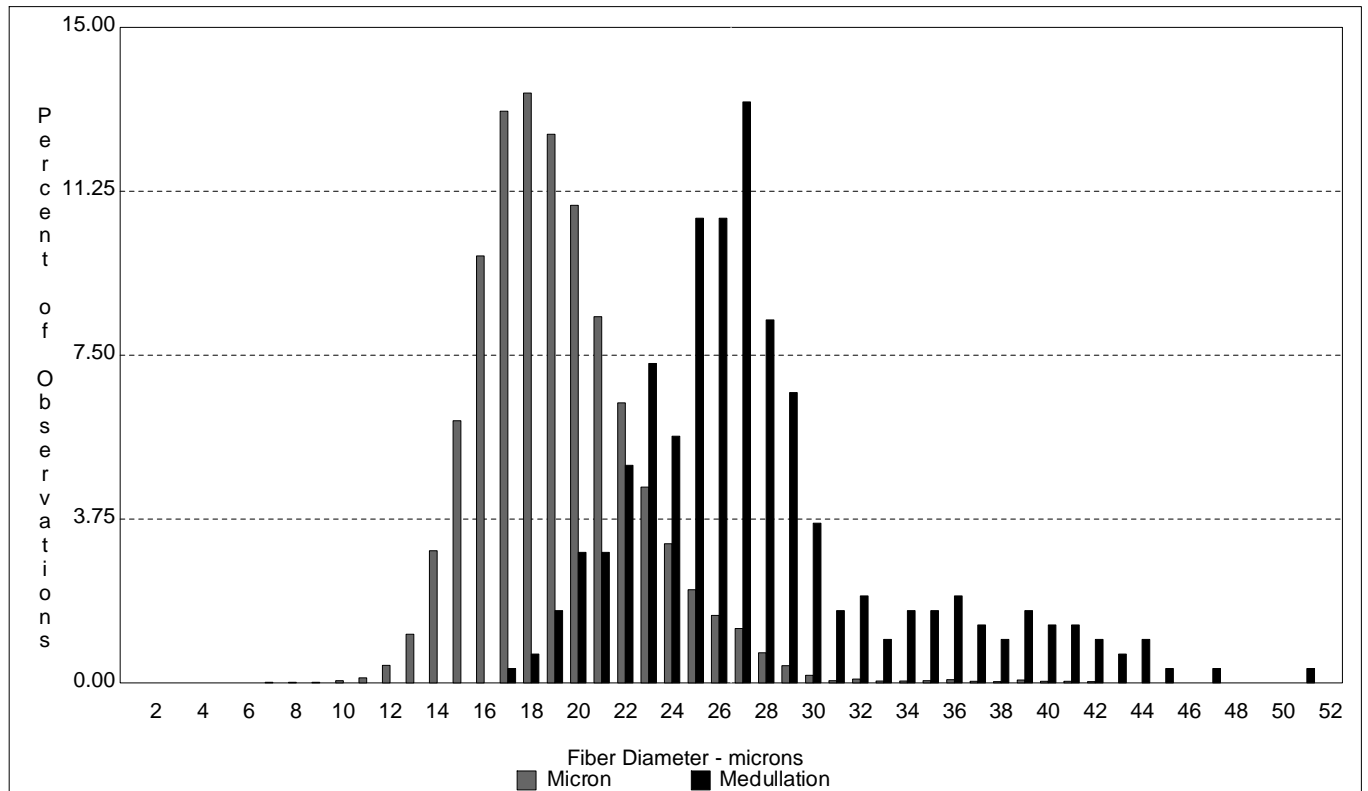

This Test Performed According to I.W.T.O Method 47