



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Rainbow Forest Acres/Barbara Eslake
PO Box 1203, 7756 Owl Ridge Rd
Mt Currie BC V0N 2K0 Canada

05/18/11

Test No: 402171


Animal and Sample Description

Animal Name: RFA Ivey
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/01/11
Age: 09/14/02

Laboratory Data

Mean Fiber Diameter:	21.2 microns	Spin Fineness:	20.4 microns
Standard Deviation:	4.2 microns	Mean Curvature (deg/mm):	48.5
Coefficient of Variation:	20.0 %	SD Curvature (deg/mm):	24.8
Fibers Greater Than 30 microns:	3.6 %	Comfort Factor:	96.4 %
Medullated Fibers:	5.6 %		

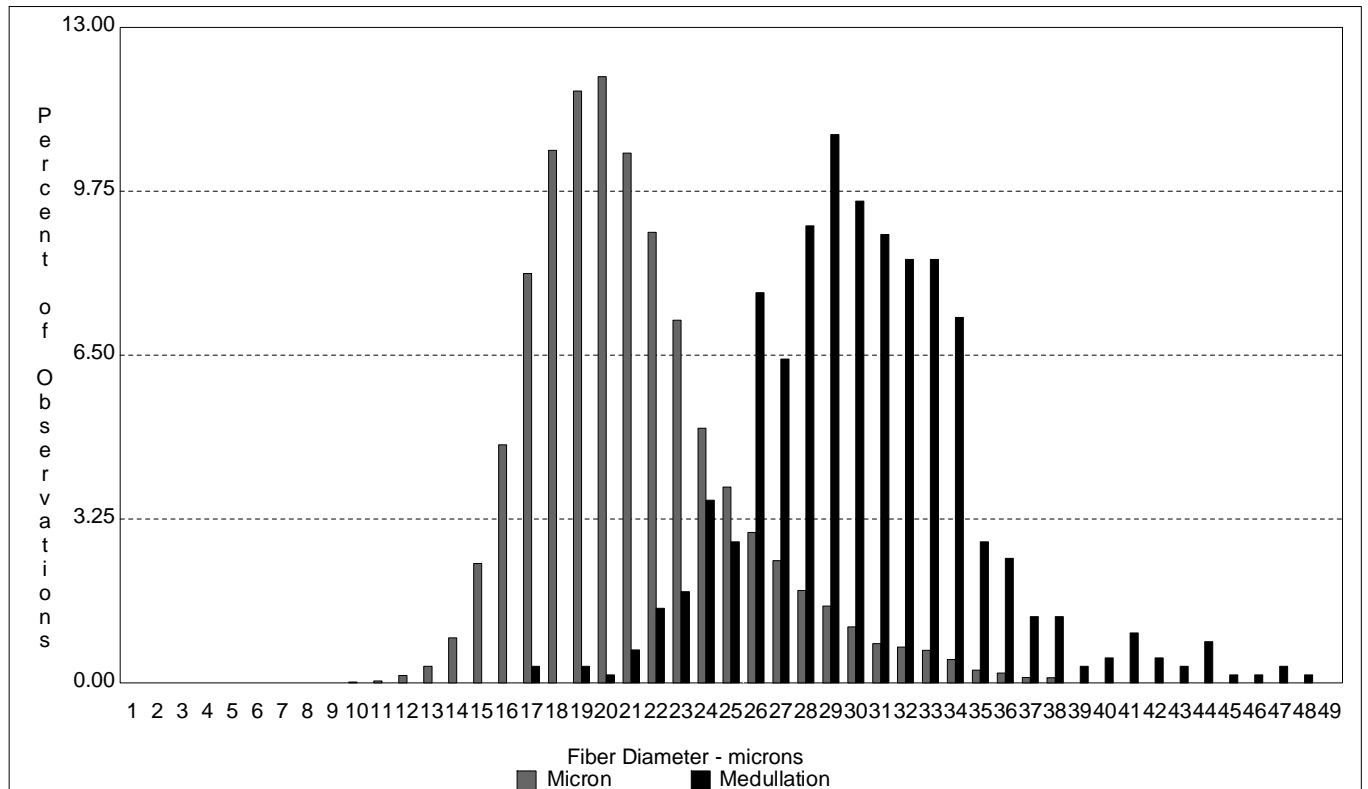

This Test Performed According to I.W.T.O Method 47